


# Prep mode rack kits for Frac-950

## Instructions


### Assembling the rack

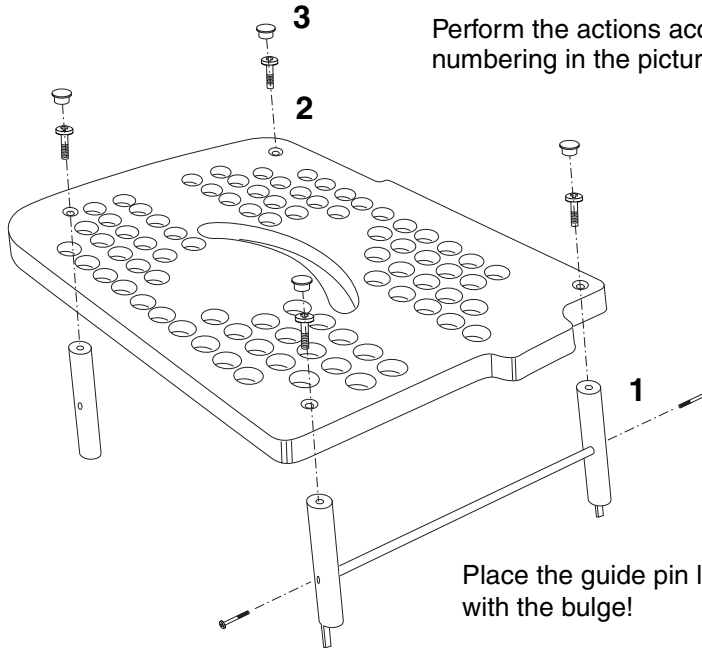

Perform the actions according to the numbering in the pictures.

Place the guide pin legs at the side with the bulge!

### Installing the rack

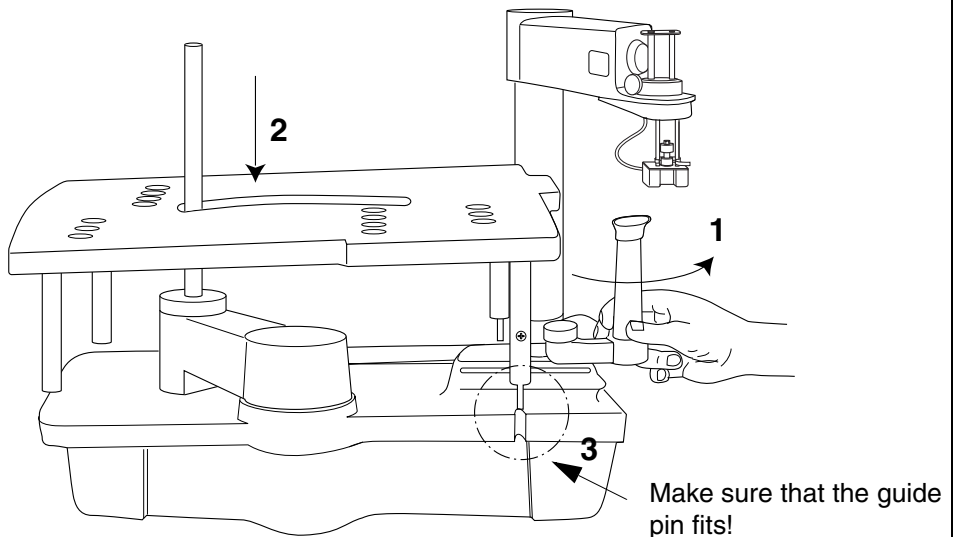

## Important user information

### Declaration of conformity

The **CE** symbol and corresponding declaration of conformity, is valid for the instrument when it is:

- connected to other CE-marked Amersham Pharmacia Biotech instruments, or
- connected to other products recommended or described in this manual, and
- used in the same state as it was delivered from Amersham Pharmacia Biotech except for alterations described in this manual.

### Terms and Conditions of Sale

All goods and services are sold subject to the terms and conditions of sale of the company within the Amersham Pharmacia Biotech group which supplies them. A copy of these terms and conditions is available on request.

Should you have any comments on this product, we will be pleased to receive them at:

**Amersham Pharmacia Biotech AB**  
SE-751 84 Uppsala  
Sweden

### Trademarks

Amersham is a trademark of Nycomed Amersham plc. Pharmacia and Drop Design are trademarks of Pharmacia & Upjohn Inc.

### Office Addresses

**Amersham Pharmacia Biotech AB**  
SE-751 84 Uppsala  
Sweden

**Amersham Pharmacia Biotech UK Limited**  
Amersham Place  
Little Chalfont  
Buckinghamshire  
England HP7 9NA

**Amersham Pharmacia Biotech Inc.**  
800 Centennial Avenue  
P.O. Box 1327  
Piscataway, N.J. 08855  
USA

**Amersham Pharmacia Biotech Europe GmbH**  
Postfach 5480  
D-79021 Freiburg  
Germany

**Amersham Pharmacia Biotech KK**  
Sanken Building  
3-25-1 Hyakunincho, Shinjuku-ku  
Tokyo 169-0073  
Japan

© Copyright Amersham Pharmacia Biotech AB 2001  
- All rights reserved